




CUSTOMER PROVIDED:

RECEPTACLES:

- OUTLET "A": Outlet, Shall be a dedicated circuit for 120 volts 15 amps for the Computer and Printer. NEMA 5-15R (AS PER LOCAL CODE)
- OUTLET "B": Network drop and telecommunication outlet
- OUTLET "C": Outlet, Shall be a dedicated circuit for the iDXA Bone Density Machine. 120 volts 15 amps. NEMA 5-15R (AS PER LOCAL CODE)

	DOUBLE RECEPTACLE OUTLET
	COMPUTER NETWORK PORT (100Mbps / 1 Gbps) AND PHONE RECEPTACLE

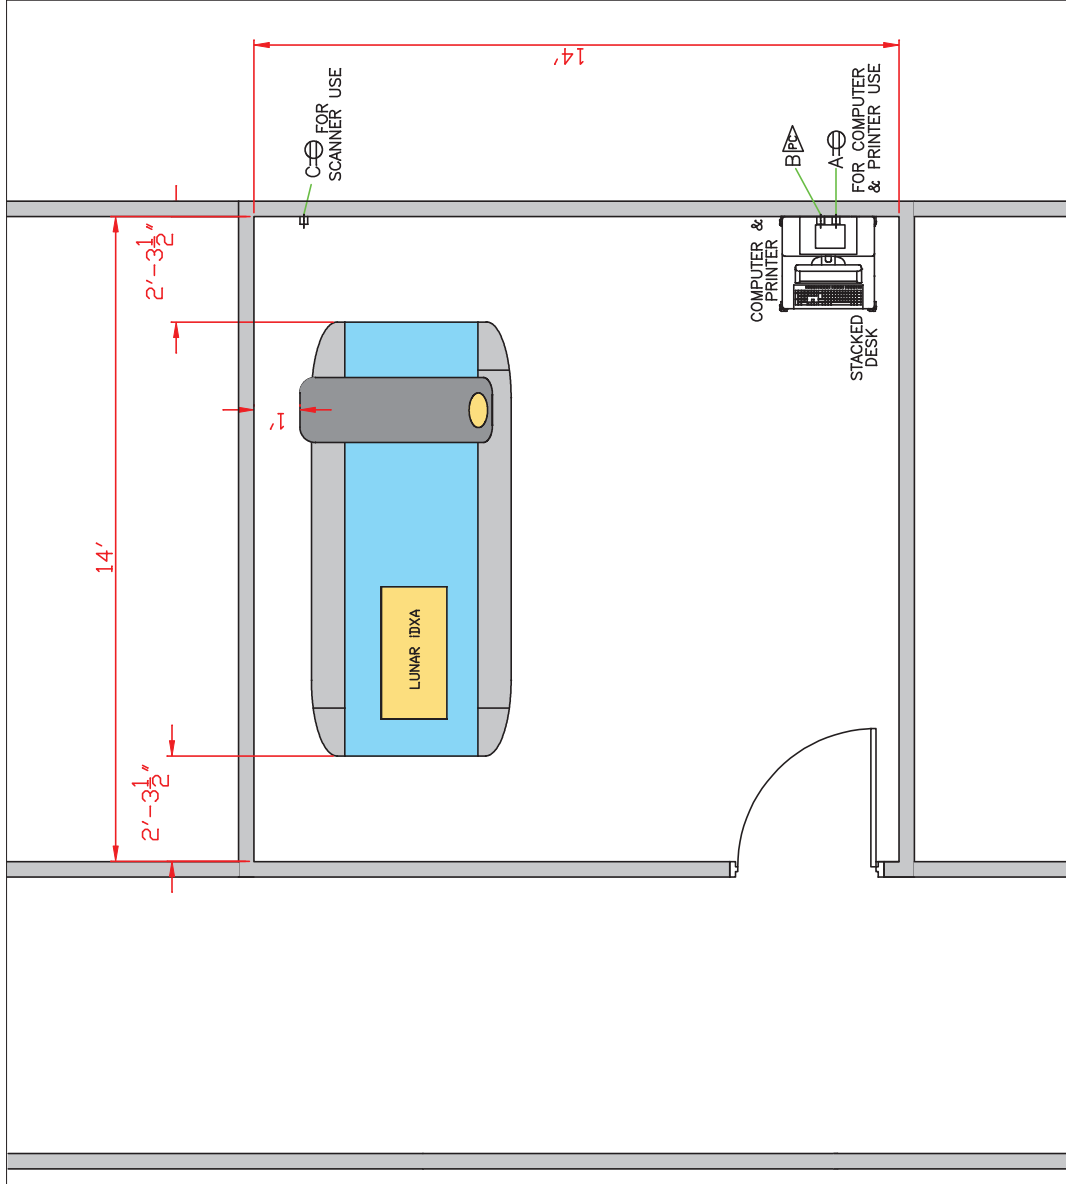

BMD ROOM

Horizon Medical Services Ltd.

iDXA BMD – ROOM PLAN

OPTIMUM SAMPLE 14' x 14' ROOM

SCALE 1:50	PHONE 1 800 267 1442	FAX 905 567 5148	SHEET 1 OF 2
SIZE A	www.horizonmedical.com j.binczarowski@horizonmedical.com Drawn by: JB Mar. 2011	DWG NO. SAMPLER20110308	REV 1

ALL DIMENSIONS = IMPERIAL
FINAL CONFIGURATION TO BE DETERMINED BEFORE INSTALL